

(Radiation Survey Meter)



TYPE: RM701N

NUCLEONIX SYSTEMS PRIVATE LIMITED

Plot No: 162 A & B, Phase II, I.D.A. Cherlapally, Hyderabad - 500 051.

Phone: 040-29706483 / 84 / 85, Mobile No: 7331104481 / 82

E-mail: info@nucleonix.com Web : www.nucleonix.com

CONTENTS


S.No.	Description	Pg.No.
CHAPTER - 1	Introduction	03-03
CHAPTER - 2	Front panel diagram & Controls indications / diagrams	04-04
CHAPTER - 3	Specifications	05-05
CHAPTER - 4	4.1. Instruction on Intelligent keypad commands 4.2. Operating Procedure	06-12
CHAPTER - 5	Calibration	13-13
CHAPTER - 6	USB to UART Data Communication & Instruction Manual for NucSoft data comm. Software	14-21
CHAPTER - 7	Availing of Maintenance / Calibration Services and warranty clause (with in India)	22-27
CHAPTER - 8	Block diagram & Description	28-28
CHAPTER - 9	CONTACT US FOR AVAILING SERVICES	29-32

CHAPTER - I

INTRODUCTION

{Radiation Survey Meter} Type: **RM701N** is a G.M. Detector based, battery powered, hand-held, general Purpose radiation Survey Meter. This will be useful for dose rate measurements in nuclear installations, Radiochemical plants, Reprocessing plants, etc. Additionally it will be useful in medical, agricultural, industrial and other installations where radioactive isotopes are used for a variety of applications. This product is designed around a Microcontroller Chip. It is provided with alpha Numeric LCD display for indicating the dose rate in digits, dose rate as a bar graph, cumulative dose in digits. It covers wide range from 0 to 10R/hr in two range with auto ranging. This unit has a facility for storing the data into built-in EEPROM along with real time. The stored data can be recalled on to the display or transmitted to PC.

Some important features of this unit:

- Conforms to ANSI N42.17A performance specifications for Health Physics instrumentation (portable) &  compliant.
- It is designed around Microcontroller Chip.
- Uses energy compensated GM Counter.
- Range change over automatic.
- Accuracy $\pm 15\%$ with CO^{60} .
- Facilitates storing recalling of readings and transmission of readings to PC.
- Works on 6V (4x1.5V) dry cell batteries.

VIEW OF (Radiation Survey Meter) RM701N



CHAPTER - II

FRONT PANEL & SIDE PANEL CONTROLS

2.1 FRONT PANEL CONTROLS AND INDICATIONS

2.1.1. LCD DOT MATRIX DISPLAY

This is a 16 X 2 alpha numeric LCD dot matrix display and responds to all the commands from the keypad and displays programme parameters like Acquisition modes (CPS, CPM, π^2 , π^2), Recall, Save etc.

2.1.2. INTELLIGENT KEYPAD

- š **Shift** This key is an important one which facilitates the user to programme the operation of the instrument for different modes/ conditions.
- > **Start** This is used for starting of acquisition once all the programme parameters have been set.
- œ **Stop** This key can be used to stop acquisition.
- Ÿ **Inc/Dec** These keys are used while setting the programme parameters to increment and decrement a value or to change the option selected to another value available.
- j **Store** This key is used for storing the readings or data values in the following way.

If you want to store the data, then press STOP button to stop acquisition and then press STORE button.

Note: Keypad commands have been explained in detail under chapter IV - 4.1.

2.2.3. POWER KEY

This is a ON/OFF button to put on the power to the unit. The power to this unit is provided through 6 volts DC, 4 x 1.5 Volts cells which is housed inside the unit.

2.2.4. TODETECTOR

LND 713 Detector placed in a energy compensated filter.

2.2.5. USB to UART (OPTIONAL AT EXTRA COST)

This connector is having USB to UART compatible signals for serial data communication to a P.C. Under software control from a P.C, the stored data reading from this unit can be down loaded on to P.C.

CHAPTER - III


SPECIFICATIONS

Detector	: GM counter Type LND 713 with energy compensated
Radiation detected	filter. : X & Gamma, from 60 Kev to 2 MeV.
Energy Response	: Within +/- 20% from 60 KeV to 1.25 Mev.
Operation Ranges	: 0-10R/hr.
Over Range	: Unit shows over range above 10R/hr to 1000R/hr.
Range Changeover	: Automatic.
Accuracy	: +/- 15% with CO ⁶⁰ :
Acquisition Modes	:CPS, CPM & mR/h, µSv/h
Display	: 16X2 alpha numeric LCD display; Digital display of dose rate and units in the first line, Bar graph or dose display in the second line.
Serial Port (optional)	: Built-in USB to UART for PC linking, along with data communication software cable.
Aural	: Built-in buzzer provided.
Data Storage	: Storage of readings in built-in EEPROM. Stored Data can be recalled on to the display or transmitted to PC.
Control Buttons	: START, STOP, PROG, STORE, INC & DEC are the six control buttons provided on the instrument. The above buttons allow the user to program & operate the instruments in appropriate manner.
Real Time Clock	: On board real time clock with battery backup keeps real time information. On selecting data storage, current real time is saved along with dose rate.
Power	: 6V DC size AA MN1500 LR6 (4x1.5) alkaline cells
Dimensions	: 106W x 196L x 85Ht in mm (approx.)

CHAPTER - IV

4.1 INSTRUCTIONS ON INTELLIGENT KEYPAD COMMANDS


When we switch on the unit, the display will show up, **Backlight** is ON till the acquisition mode is executed.

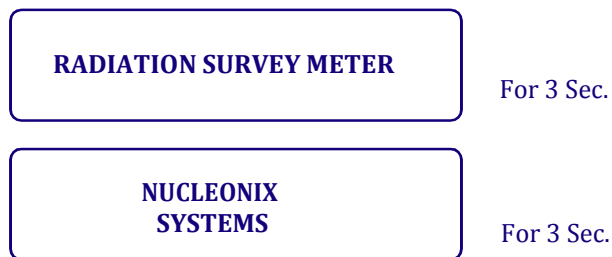


Note : **Backlight** for this unit is ON for about 6 seconds on operation of any key.

4.1.1 ACQUISITION MODE SELECTION

By default, it will be in Dose rate mode and it will acquire in mR/hr mode

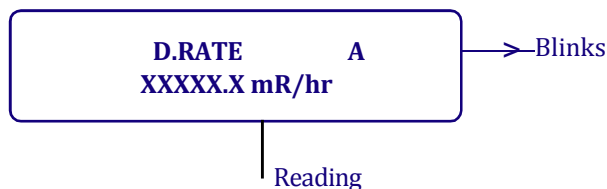


User can straight away measure the contamination in CPS / DOSERATE.



If user wants to change to other modes than the default selection then press STOP key to notice that blinking "A" vanishes and display appears as,




Now by pressing PROG key, display changes to



For changing ACQ MODE to different modes, user can change the mode by using ▲ or ▼ keys to change the mode to CPS, CPM, mR/h & μSv/h


4.1.2 ACQUIRE IN CPM MODE




If user wants to acquire contamination in CPM mode he can now stop the acquiring of contamination by pressing STOP key and press PROG key once again, display appears as follows.

ACQ MODE
mR/h


Now press ▲ or ▼ keys to change the mode to CPM.



Having selected CPM mode one can acquire the dose rate in CPM mode by pressing START key




Now display appears as,




CPM A → Blinks
XXXXXX

It will indicate CPM with time constant of 5 seconds, to stop the acquiring of contamination press STOP key




By pressing PROG key, display changes to



ACQ MODE
CPM


4.1.3. ACQUIRE IN CPS MODE




If user wants to acquire contamination in CPS mode he can now stop the acquiring of contamination by pressing STOP key and press PROG key once again, display appears as follows.

ACQ MODE
mR/h


Now press ▲ or ▼ keys to change the mode to CPS.




Having selected CPS mode one can acquire the dose rate in CPS mode by pressing START key




Now display appears as,



CPS A → Blinks
XXXXXX




It will indicate CPS with time constant of 1 second, to stop the acquiring of contamination press STOP key



By pressing PROG key, display changes to

ACQ MODE
CPS

4.1.4. ACQUIRE IN DOSE RATE MODE




Now press Increment or Decrement keys to select DOSE RATE in mR/h

ACQ MODE
mR/h

This mode is selected for Gamma Dose rates upon 10R/hr.

4.1.5. SETTING OTHER PARAMETERS


Press PROG key to select the required parameters. By pressing PROG key, display changes to



ACQ MODE **mR/h**

If one presses PROG key, then the option changes from ACQ MODE to other option as follows

4.1.6. STORED READINGS:




STORED
READINGS **XXXX**


STORED READINGS: This displays the number of readings stored in unit.

4.1.7 SETTING ALARM SET POINT:


Having selected preset time, user needs to enter the preset time for which he intends to acquire. He can be do so by first setting ACQ mode to Dose rate/count rate mode.

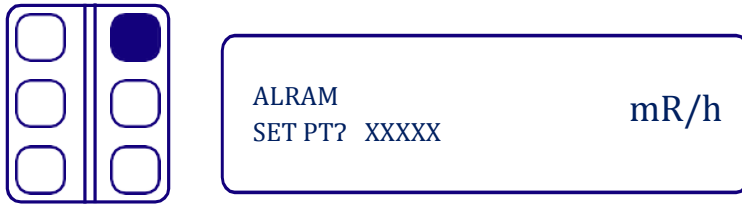

Now using Increment or Decrement buttons Alarm set time can be adjusted.




Now using increment or decrement buttons we can adjust the alarm setpoint time in the range of 0-99999 CPS/ 0-99999 CPM / 10000.0 mR/hr, 100000 μ sv/hr.



4.1.8 PASS CODE: This is a very useful & important feature, it allows one to enter the calibration factor to obtain expected dose rate. Since the unit is calibrated at factory, user is advised not to disturb the calibration. This is to be changed only if user intends to re-calibrate the unit.



If you want to change the Calibration factor, use increment or decrement keys set for PASS CODE 90. Then press PROG KEY to change the calibration factor, then the display will appear like this. By using the keys

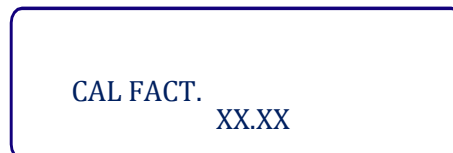

4.1.9 BUZZER: On pressing PROG key the following display appears,




The default buzzer condition is OFF. User can change this by pressing increment or decrement keys




4.1.10 RECALL DATA READINGS:

This is a very useful feature that has been provided in this unit. At the end of storing / saving of a set of readings, this feature will enable the users to recall the readings on to the display

By pressing PROG key, display changes to,

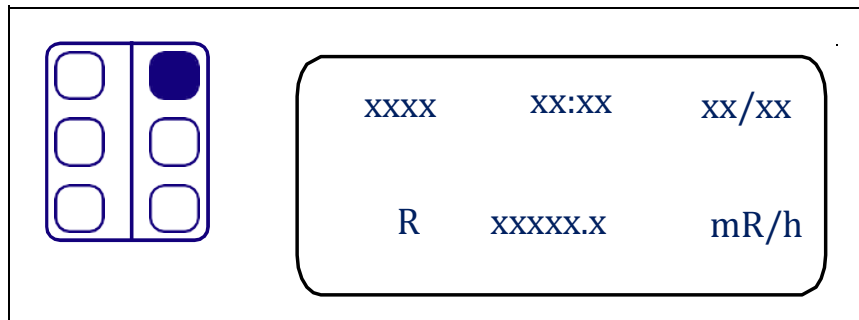


Recall the stored data in serial wise by pressing increment or decrement

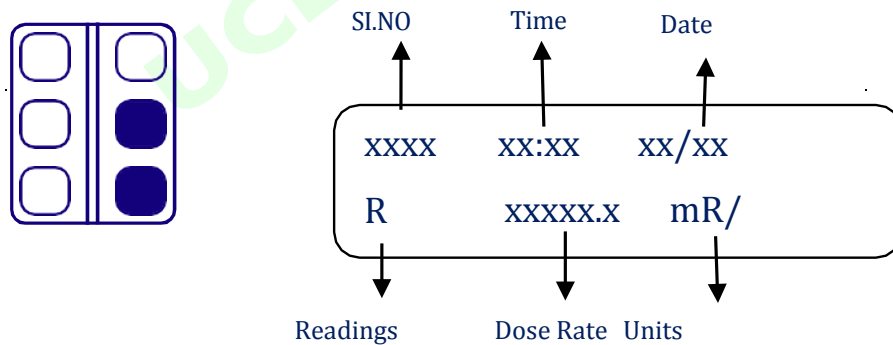


4.1.11 ERASING THE PROGRAMME PARAMETERS:

ERASE MEMORY?


To erase stored values press Increment or Decrement keys.



"OK" will be displayed on erasing parameters (PROG)




4.1.12 REAL TIME CLOCK (RTC):




RTC xx:xx XX/XX

User can change date and time by using the increment or decrement




4.1.13 BACKLITE CONTROL:




BACKLITE ON

This is having two option as ON and OFF .we can select by using these increment or decrement keys.




4.1.14 SAVING PROGRAMMED PARAMETERS:

All the programmed parameters are to be saved by the user before he can start acquisition. Without saving, the system will use the previous parameters for acquisition. By pressing PROG key, display changes to,



SAVE? (PRG)




To save the above parameters press Increment or Decrement keys. "OK" will be displayed on saving of parameters (PRG).


4.1.15 STORING OF DATA READINGS:

This system has CMOS memory to store up to 1000 readings. To store any data use the following procedure.

Press STOP key to stop acquisition.



Then press STORE key to store the current data or readings ,and the Sl. No in the display increments to the next value.



MENU	OPTIONS
ACQ MODE	DOSE RATE,CPS,CPM
STORED READINGS	XXXX
ALARM SET PT?	XXXXXX μ Sv/h
PASS CODE	90
CAL. FACT	XX.XX
BUZZER	ON/OFF
RECALL DATA	-
ERASE MEMORY?	-
RTC	XX.XX XX/XX
BACKLITE	ON/OFF
SAVE?(PRG)	-

4.2 OPERATING PROCEDURE:

1. This unit is packed and dispatched in ready to use condition. On unpacking, user is advised to go through Instruction Manual including instructions under Chapter IV (4.1) completely.
2. Now switch ON the power to the unit by pressing the Rocker switch to the ON position.
3. User can now operate the equipment to make measurements in CPS/CPM or DOSERATE modes as per the requirement. User can store and recall the readings if required also.
4. Optional feature(offered against specific order only) :
Stored readings can be downloaded into a PC if required under the control of data communication software which is supplied at extra cost as an optional accessory.

CHAPTER -V

CALIBRATION


PRE CALIBRATION

This unit is already having a micro-controller loaded with look-up table containing calibration data (i.e., cps Vs dose rate tables). In pre-calibration, one can check by feeding tail pulses to the unit after isolating the detector from the circuit. Unit display indication will show corresponding dose rate which should confirm to the look-up table data. However each unit may require certain amount of recalibration check in the presence of source calibration is given in the following paragraph.

SOURCE CALIBRATION

This unit namely **Radiation Survey Meter Type : RM701N** has been calibrated at Radiation standards and calibration Lab (RS & CL) of Nucleonix Systems (P) Ltd., situated at their works.

Before calibration with source, set the calibration factor to 1.000 & save the settings. No select R/hr as unit of measurement of dose rate. Now place the instrument in the source beam such that detector is perpendicular to the beam axis as shown in below figure.

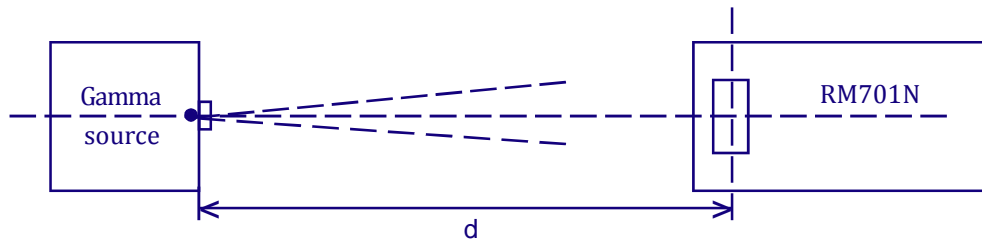

S.No	Expected Doserate	Observed Doserate
1	1 mR/hr	
2	10 mR/hr	
3	20 mR/hr	
4	100 mR/hr	
5	1 R/hr	
6	2 R/hr	
7	5 R/hr	
8	10 R/hr	
9	15 R/hr	
10	20 R/hr	

Note: CRC - 2 camera having CO⁶⁰ standard supplied by B.A.R.C Mumbai.

The observed doserates have been to be written +/-15% of the expected doserates for CO⁶⁰

In case they do not fall within the expected accuracy, then adjust calibration factor so that entire readings will be within +/-15% of expected doserates.

Once calibration factor is set, make below measurements.

In these readings are found to be within +/-15%, then expected doserates then unit calibration is said to be complete.

When the manual is dispatched to the customer, calibration factor is to be mentioned below and also saved in the instrument program.

Note: This instrument will show the constant reading above the 10 R/hr indicating the OVR in the 16x2 Display upto 200 R/hr.

Over Load test passed:

- | | | |
|-----|-------------------------|--------|
| (a) | 10 times highest range | Yes/No |
| (b) | 50 times highest range | Yes/No |
| (c) | 100 times highest range | Yes/No |

Calibration Factor : _____

Probe Type : _____

Calibration Date : _____

Calibrated by : _____

Calibration Due : _____

Instrument S.No. : _____

CHAPTER – VI

USB to UART DATA COMMUNICATION & INSTRUCTION MANUAL FOR NUCSOFT DATA COMMUNICATION SOFTWARE

1. Put the CD in CD Drive and open the CD by clicking mouse button.
2. Automatically, it will go through set-up procedure for the mRLink.
3. By selecting mR link, PC down load software for NX-Instruments will appear on the monitor. In that screen one would see Port setting & Data setting options.
4. Select appropriate Port setting and give the port number
5. Select Data setting to give start Sl.No. and Number of readings, to be down loaded from the instrument inDto PC.
6. Now log the data, by clicking on the Log data button the monitor will show up Serial Number, Label and Counts / Count rate / Doserate information on the display.
7. Enter the Nucsoft ID .& PWD as


I D: admin
p swd:Nucleonix

INSTALLATION PROCEDURE


The following is the procedures to install NUCSOFT. Please follow the steps

→ please insert the NUCSOFT CD in the CD drive


→If not then explore the CD and double click on "nucSoft"

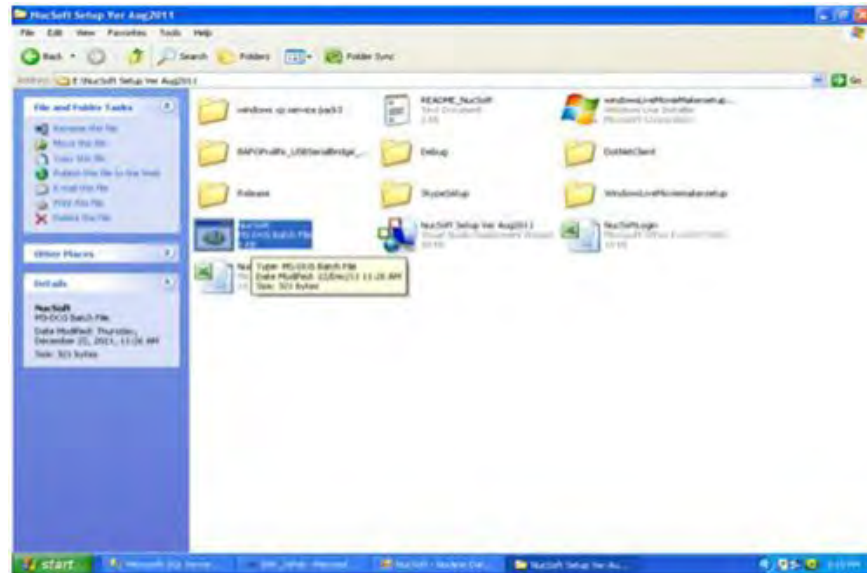


- If .NET is not there in your system you have install the .NET software.
- Following window appear for installing .NET

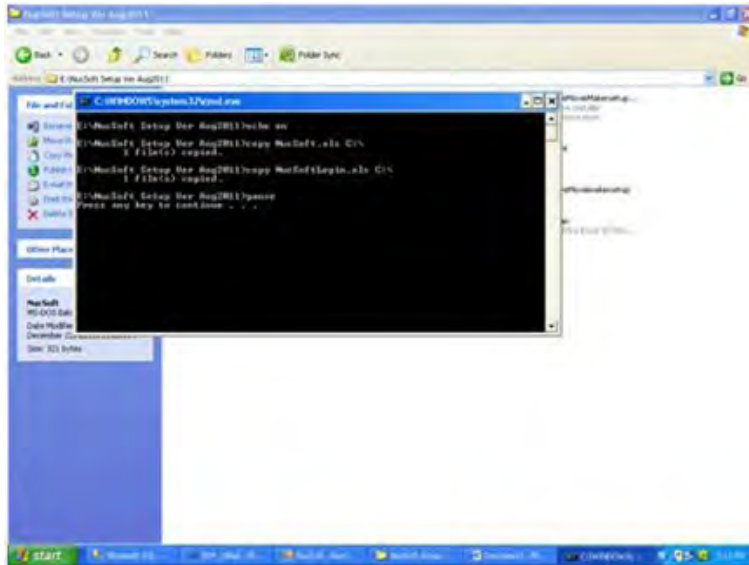

- Press any key from keyboard the installation will start and the following window will appear

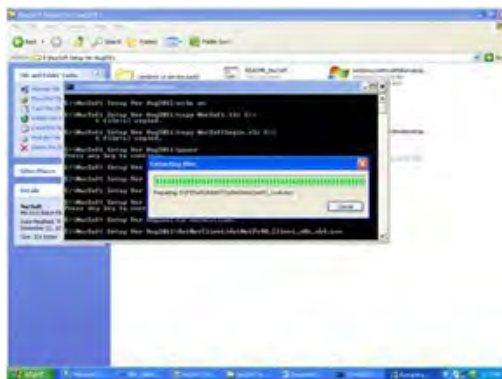


Click

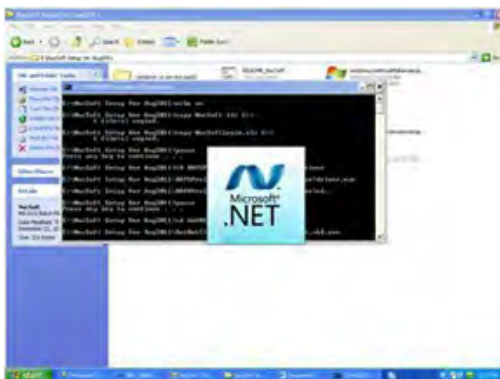


Click on computer symbol


→ Follow the installation procedure. When following screen appear click continue

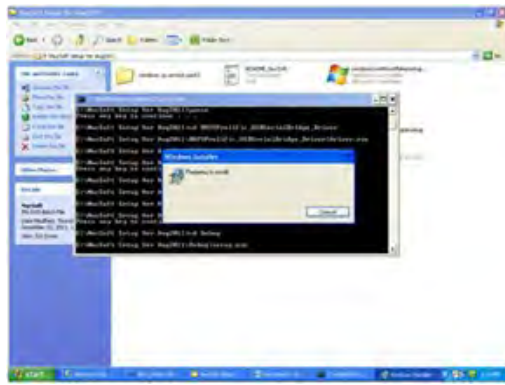


→ Follow screen will appear several times, each time click yes

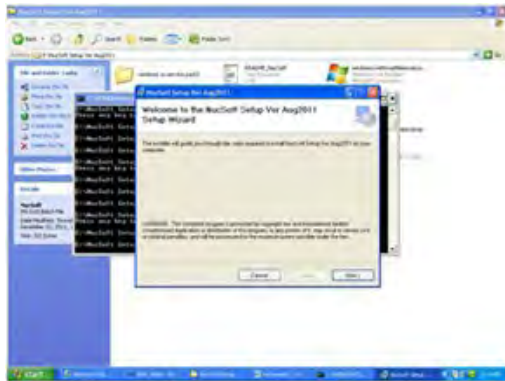

→ If following screen appear then click on "ignore" then click OK.

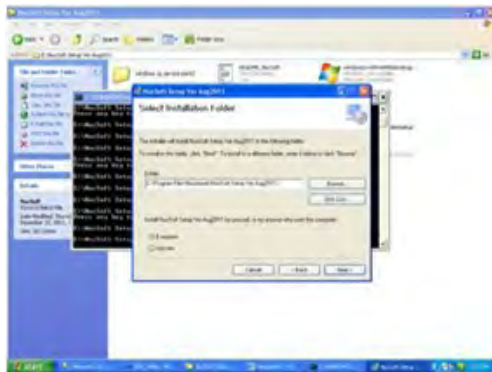


→ Click OK on following screen. Installation complete successfully

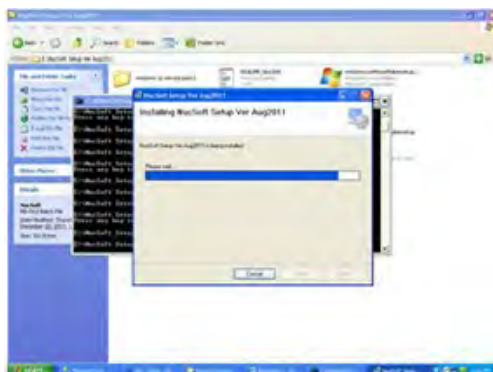


→ Installation complete successfully. You can check by clicking NucSoft then you have to enter the given user name and password.


→ Enter user name and password

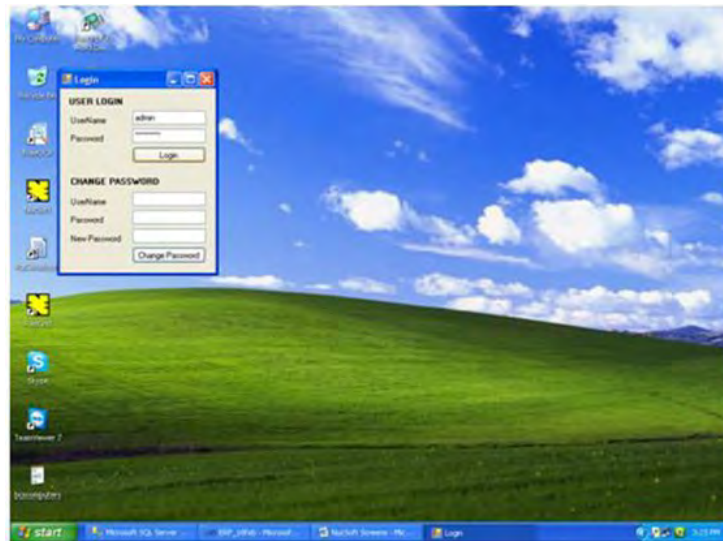


→ After entering the user name and password the screen appears like this. Now you have to configure the comm. port and baudrate.

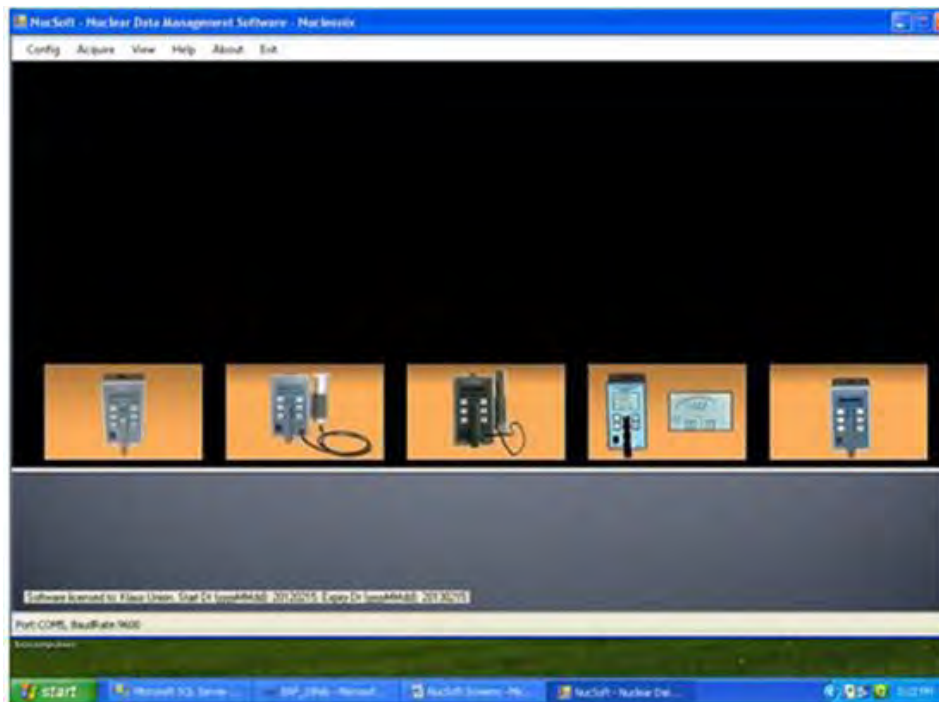


→ Now you can see the following screen. Now you can enter the COM port number in the given slot as "1" and press OK.

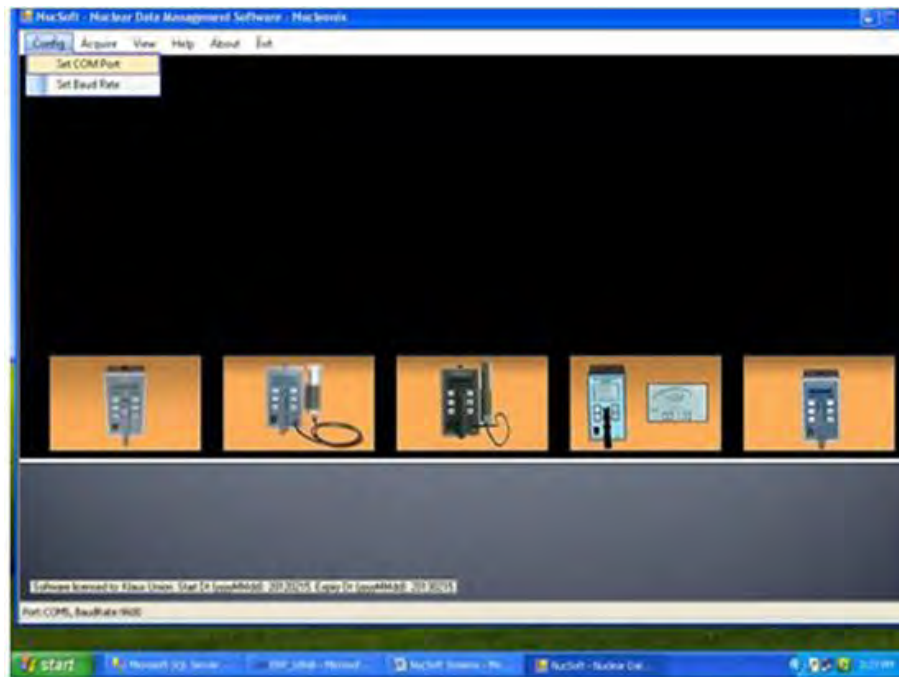


→ Now you can see the following screen. Now you can enter the baud rate number in the given slot as "9600" and press OK.

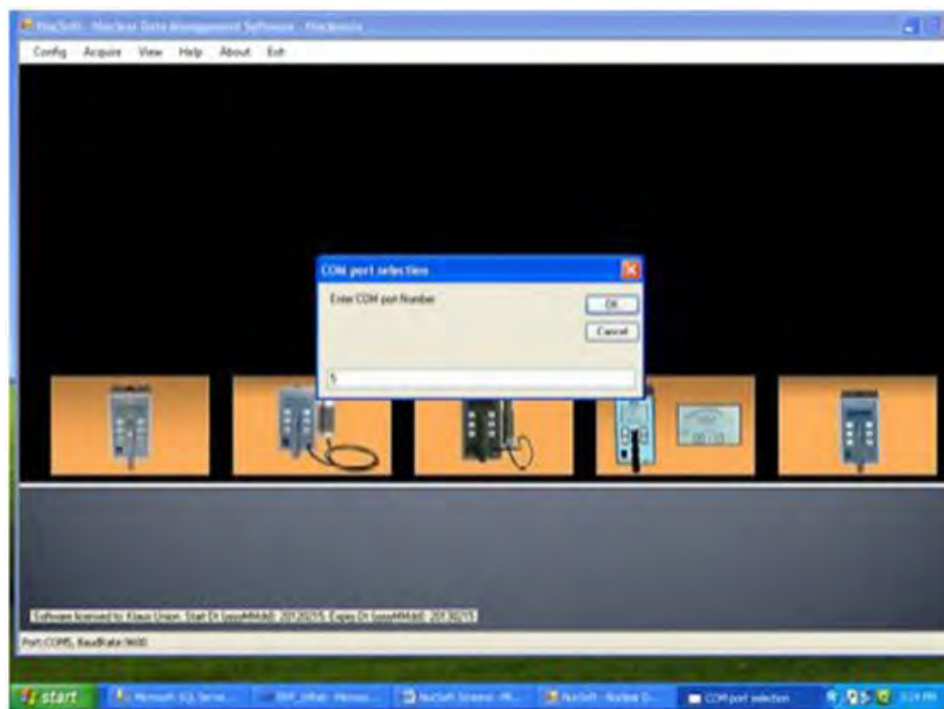

→ After pressing the Acquire it show that is downloading data.

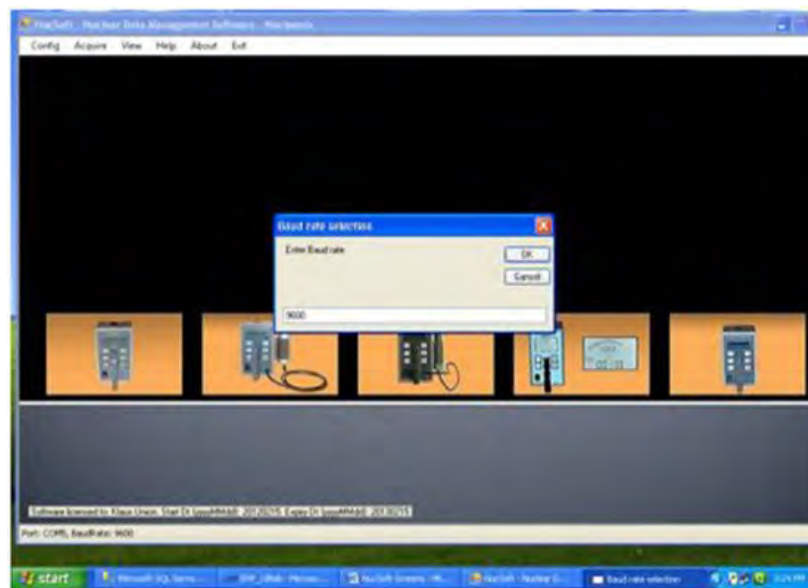

→ After that you can see the following screen. You have to acquire the data.

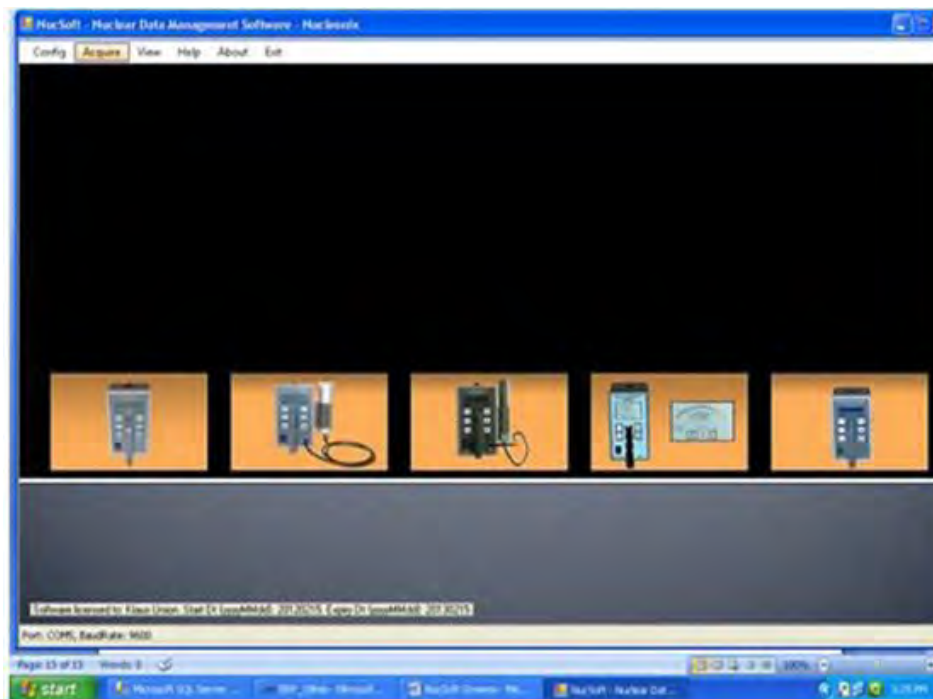

→ After acquiring data the screen appears as we have stored the data in the unit. The reading can be displayed like this MSEXL format.

G38									
	A	B	C	D	E	F	G	H	I
1									
2		SL.NO	LABEL	TIME	DATE	BG_READING	ALRM_SET_PT.	MEASURED_VALUE?	
3		1		67 17:32	16/12	00014.6uR/h	00081.2uR/h	00017.4uR/h	
4		2		67 17:32	16/12	00014.6uR/h	00081.2uR/h	00018.4uR/h	
5		3		67 17:32	16/12	00014.6uR/h	00081.2uR/h	00016.4uR/h	
6		4		67 17:32	16/12	00014.6uR/h	00081.2uR/h	00018.0uR/h	
7		5		67 17:32	16/12	00014.6uR/h	00081.2uR/h	00018.4uR/h	
8		6		67 17:32	16/12	00014.6uR/h	00081.2uR/h	00017.4uR/h	
9		7		67 17:32	16/12	00014.6uR/h	00081.2uR/h	00019.0uR/h	
10		8		67 17:32	16/12	00014.6uR/h	00081.2uR/h	00019.0uR/h	
11		9		67 17:33	16/12	00014.6uR/h	00081.2uR/h	00019.6uR/h	
12		10		67 17:33	16/12	00014.6uR/h	00081.2uR/h	00019.6uR/h	
13		11		67 17:33	16/12	00014.6uR/h	00081.2uR/h	00015.4uR/h	
14		12		67 17:33	16/12	00014.6uR/h	00081.2uR/h	00018.6uR/h	
15		13		67 17:33	16/12	00014.6uR/h	00081.2uR/h	00017.6uR/h	
16		14		67 17:33	16/12	00014.6uR/h	00081.2uR/h	00016.2uR/h	
17		15		67 17:33	16/12	00014.6uR/h	00081.2uR/h	00016.2uR/h	
18									

→ You can view the reports as follows. You can also take the print by clicking print option on the tool bar. By this the report generation is over.

CHAPTER - VII

AVAILING OF MAINTENANCE/ CALIBRATION SERVICES AND WARRANTY CLAUSE (with in India)

7.1 GENERAL

As per the warranty clause of the company we provide one year warranty during which period we provide free service at our works. Hence in case of any mal-function in our instruments you are requested to send the unit back to our works by RPP/COURIER/SPEEDPOST/PARCEL/GATI/XPS/door delivery. We shall arrange immediate rectification/replacement within two weeks from the date of receipt of the equipment at our place. Please note that the equipment will be serviced at our works only.

The equipment is to be sent to:

The Servicing Department

NUCLEONIX SYSTEMS PRIVATE LIMITED

Plot No: 162 A & B, PHASE II, I.D.A. Cherlapally, Hyderabad - 500 051

Phone: + 91-7207034546, 68888777, Mobile: 7331104480, 7331104481, 7331104482

E-mail: info@nucleonix.com www.nucleonix.com

For all the Radiation monitoring equipment, detectors built-in or external probes will not have one-year warranty, only inspection warranty at the time of supply is provided. Since detectors will / may have fragile glass construction we do not provide warranty. In case of failure of these components at cost price as per Nucleonix price list user has to buy.

Note: In respect of all types of portable radiation monitors, it may be necessary to checkup and recalibrate the equipment once a year at our works.

7.2 EQUIPMENT REPAIRS / SERVICING POLICY (WITH IN INDIA)

7.2.1 DURING WARRANTY

The following procedure is to be followed by the customers with in India for availing services/ repairing facility during warrantee period.

Equipment's are to be sent to our works for availing free repair services during warrantee, after the customer receives approval from the customer support division, by sending an e-mail.

For all equipment's, costing less than 6.0 lakhs one year warrantee & free service is offered, when the equipment's are sent to our works only. For larger systems such as installed systems, networked systems, specialized systems, costing more than 6.0 lakhs during one year warrantee, free service is offered at site. Field service Engineer will be deputed subject to warrantee terms & conditions.

This does not include personal computer related problems, for which local computer service provider of the PC vendor is to be contacted. Also for software related problems online support will be provided. Software support doesn't include cleaning of virus problems etc.

When the equipment's are sent to our works for warrantee services, they are to be properly packed with adequate cushion to prevent any transportation damages. Nucleonix Systems is not responsible for damages or loss during transportation.

Packing / Freight charge is to be borne by customer when he sends the equipment to our works. However when we return after servicing packing will be Nucleonix responsibility & Freight charges will be to your account. Only services are free.

Please indicate in your correspondence equipment model & serial number.

All the equipment's are to be sent to our works only on door delivery basis.

For Door Delivery Transportation contact XPS/GATI cargo in your city / town or a reliable courier service to pick the consignment from your place. For their nearest local address & phone no's look into their websites. Transit insurance if the customer feels is necessary it is to be covered.

Nucleonix Systems will not receive the equipment's sent by other modes of transportation, such as Rail/Road.

After servicing, equipment's will be sent back by same mode of transport such as XPS/GATI/COURIER/ RPP.

All types of Radiation detectors, glass ware, PMTs etc. which are fragile are not covered in warrantee, if the failure is due to physical damage, external or internal due to shock, dropping, miss-handling etc. If the failure is due to a natural fault then only it is covered under warrantee for a limited period of three months. However complete electronics is covered for 1 year warrantee.

You can also send the equipment personally to our works for repairs either during or after warrantee, after fixing up with our service dept (Customer Support Division). If possible we may repair on same day or your person can stay for a day or two & get it repaired & or calibrated.

7.2.2 AFTER WARRANTY SERVICES

On expiry of 1yr warrantee if you like to send the equipment (low cost less than 6.0 lakhs) for repairs to our works, you may please observe the following procedure.

Send an e-mail with details mentioning that you agree to pay service charges which includes: Basic service charges per unit / module in the range of Rs: 2500 to Rs : 10,000 depending on the sophistication of the unit calibration charges (if applicable for your equipment) + cost of components + packing charges + Return Freight charges @ actual.

Once our customer support department responds & requests you to despatch the equipment to our works for repairs, you may do so by following the steps given below.

Followed by this you can send the equipment straight away if it is within 5 yrs old. If the equipment is beyond 5 yrs old, then also you can send it for repairs, however only after you receive confirmation from Customer Support Division, that it is repairable & is not an obsolete model. If the design is obsolete then customer support division (CSD) may give you 'buy back' offer to replace with new model or upgrade it with electronic circuit boards & enclosure.

For all installed equipment's costing above Rs: 6.0 lakhs which are larger in size & for which field servicing only is recommended, you can obtain a quotation with relevant details by sending an e-mail & avail the services accordingly.

For all field servicing jobs, since we need to depute engineers, it is likely, to take time & also it will cost more which includes Engineer's TA& DA etc., apart from basic service charges + cost of spares etc. Please note that basic service charges will be different for different products depending upon sophistication.

Also in some cases it may not be possible to fix-up the problems in the field itself, in such cases we may advise you to send them to our works.

For all jobs to be serviced in the field, customer is requested to provide adequate details on the nature of problems, to enable our engineer to come prepared with adequate spares.

For any additional information send an e-mail to info@nucleonix.com, Atten: Customer support division.

7.3 EQUIPMENT REPAIRS / SERVICING POLICY (FOR EXPORTS)

Equipment's, manufactured & exported are subjected to a well defined quality assurance (QA) plan & Factory acceptance tests (FAT). Nucleonix systems has the following policy to provide maintenance support to overseas customers either directly or through international dealers/ distributors.

(a) During & after warranty:

For minor problems, which can be handled by customers, servicing tips have been provided in the user manual / servicing manual.

Also most of the equipment's have built-in fault diagnostic features which will indicate to the user nature of problem in the equipment. Based on the visual indication in the instrument Display, user can take corrective action or contact Nucleonix systems by email for help.

Nucleonix systems will guide in localizing the defective part / module or sub-system by interacting with the customer if required. Skype will be used for communication.

During warranty free replacement of sub-system or board (PCB) will be done. However customer has to send defective sub-system back to Nucleonix system with-in 15 days on arranging replacement.

During & after warranty, any Freight charges & customs clearance charges are to be borne by customers, both ways.

If it is a manufacturing defect, then Nucleonix system will bear the replacement cost of sub-system / unit. However any Freight charges & customs clearance charges in their country are to be borne by customer. After warranty, services will be similar to that of services during warranty. However, customer will have to pay for cost of parts replaced, freight charges both ways & customs clearance charges in both the countries. Nucleonix systems plans to introduce audio visuals on web or on CDs to facilitate product demonstration, installation & minor maintenance very soon.

7.4 HOW TO AVAIL CALIBRATION SERVICES (FOR INDIAN CUSTOMERS)

Nucleonix Systems offers radiation calibration services to its customers. Calibration services are provided for Nucleonix Systems manufactured products only, in general, as a company policy.

How to avail calibration services:

It is best advised that each of the Radiation monitors including Area monitors are calibrated once in a year. When you want to send your Radiation monitor / Area monitor / Contamination monitor for calibration to our works. You may send the equipment for calibration, by following the steps given below:

1. Our standard calibration charges per equipment (All types of Radiation monitors including portable survey meters, contamination monitors & Area Gamma Monitors) are Rs: 2500 + Packing + Freight charges. You can email a 'work order' accepting these charges.
2. Email your work order and despatch / send the equipment to our works if it is 5 years old or less including details of mode of transport sent with docket particulars.
3. Also mention in your work order & clearly indicate that you will agree to pay calibration charges & also equipment repair charges additionally if the unit is faulty & requires repairs before one can take it up for calibration.
4. You are requested to ensure good packing to avoid any transportation damages. Especially if there are external detector probes, they are to be packed with sufficient soft foam to ensure no damage in transportation.
5. Use only the specified following mode of transportation system for dispatching on door delivery basis. XPS/GATI cargo/ Courier/RPP/Speed Post parcel etc. Send the equipment on freight paid basis. (Equipment's sent by other methods such as Rail/Road etc will not be collected). Also you can cover for transit insurance both ways if you wish. Nucleonix system is not responsible for any transportation damages or loss during transportation both ways.
6. Immediately on receipt of the equipment, we will send an acknowledgement & also a proforma bill by email/post.
7. Based on the proforma bill, once we receive the payment, equipment will be dispatched back by similar mode of transportation as mentioned above.

7.5 HOW TO AVAIL CALIBRATION SERVICES (FOR FOREIGN CUSTOMERS)

Foreign customers can calibrate Nucleonix make Radiation monitors/equipment's in their country at any of their accredited Radiation calibration labs. Nucleonix systems will be happy to provide any help and guidance if needed, for calibration. Alternatively if you send the equipment here to India we can also provide calibration services.

CALIBRATION STANDARDS LAB & FACILITY:

We have two calibration labs. (1) Low level Calibration Lab (2) High Dose Rate Calibration Lab


(1) Low level Calibration Lab: This has a Cs-137, 165 MCi standard. "Gamma Survey Instruments Calibration" from Amersham.

This has NIST Traceability Calibration of all portable radiation monitors, survey meters, contamination monitors, Area monitors etc., is carried out in this lab up to 1R/hr max dose rates.



Gamma Survey Instruments calibration has Cs-137 source 161.5 mCi as on 5th Aug 2002. It is basically a Gamma Survey Instruments calibrator procured from AEA Technologies UK/USA. Has NIST traceability within +/- 7%.

- (2) **High Dose Rate Calibration Lab:** This lab has a 8Ci, Co-60 standard housed in a CRC-2 camera, operated remotely viewed through CCTV arrangement. High dose rate survey meters, High level Area monitors etc are calibrated in this lab. This CRC-2 camera is housed in a separate concrete building. All the radiation monitors manufactured by Nucleonix Systems are authentically calibrated at this facility, before they are shipped / dispatched.

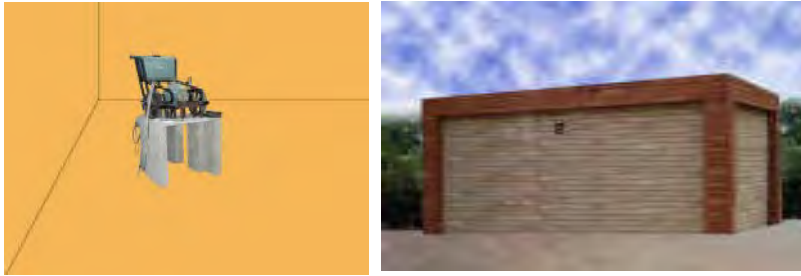

CRC-2 camera has Co-60 standard obtained from Bhabha Atomic Research Centre, Mumbai. It is a certified source.

7.6 ANNUAL MAINTENANCE CONTRACT (AMC)

Annual maintenance contract (AMC) services:

For all sophisticated instruments & systems and also for installed monitors & networked systems in a nuclear facility or a Radiological lab or in a Medical cyclotron facility where no. of instruments are networked, it is advised that customer enters into an economical Annual maintenance contract with Nucleonix system.

Detailed AMC proposal can be obtained from our customer support division (CSD), by giving required inputs.

Inputs required by our CSD to send you AMC proposal:

- 1 Name, year & data of purchase, Sl. Nos. of equipment's, Model No's, No. of equipment's for which AMC is required. Additionally no. of calls per annum required for preventive & breakdown maintenance may also be indicated.

Advantage of entering into AMC:

Equipment services offered will be prompt & timely

Nucleonix systems maintain required spares, spare tested PCBs, detectors & other critical components which may become obsolete.

Obsolescence in electronics is quite rapid. If you enter into AMC guaranteed service for the period of AMC will be the responsibility of Nucleonix Systems.

Nucleonix Systems will maintain Engineers at your disposal to attend to AMC calls on time

Without AMC prompt service calls are not guaranteed.

If some critical components become obsolete, then Nucleonix systems may request you to upgrade the product with new model or new electronics which may be expensive if you are not under AMC.

Training on maintenance / servicing:

To a limited extent, we offer training on maintenance / repairs at our works to customers on chargeable

basis. Details can be obtained from our customer support division, by customers who may require such services.

HOW TO REPLACE BATTERY

When you observe battery low voltage indication 'LB', on left corner of LCD display, it is advised that the battery be replaced to ensure correct calibration and indication of the dose rates.

Follow the below procedure for replacement of battery

- a) Lift the two latches and disengage the top unit from its bottom cover. Now holding the bottom cover lift off the top unit by its handle. (Steps 1 & 2)
- b) Notice battery holder on the bottom side of instrument electronic unit cover for battery holder is to be removed by unscrewing holder lid screws. (Step 3)
- c) Now the existing batteries mounted in the **battery holder** are to be removed and replaced with new set of batteries ensuring proper polarity. (Step 4 & 5)
- d) Now check battery voltage again, for that switch 'ON' the unit and see that 'LB' is not displayed on LCD display.
- e) Now assemble back the top unit in its bottom cover and close the unit using the latches provided.



Step-1

Note: To separate the top instrument panel with handle which also contains electronics PCB, from the bottom cover follow the instructions given below;

- A. Hold the latches both sides as shown in the above figure with thumbs touching onto the top of latch and first finger touching on to the bottom of the latch.
- B. Now bottom of the latch should be pulled outwards by using first finger as indicated in figure, by arrow.
- C. This will loosen in the latches, facilitating one, to separate the top instrument panel with handle, from the bottom enclosure of the unit.




Step-2



Step-3



Step-4

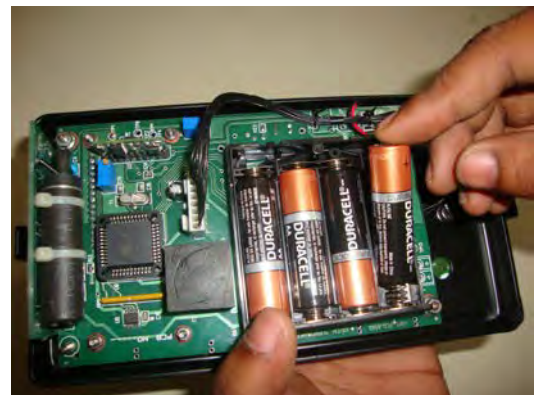

Step-5


CHAPTER -VIII

BLOCK DIAGRAM DESCRIPTION

(Radiation Survey Meter) Type: RM701N is designed around a eight bit micro-controller. Low voltage supplies, to the circuit are provided from the output of a low dropout regulator chip, which receives 6V (1.5Vx4 cells).

A compact blocking oscillator based HV circuit generates +500V required for biasing of the detector. Tail pulses generated from the GM detectors in the presence of radiation field, are converted to TTL pulses by the pulse processing circuits. These TTL pulses are fed to a serial counter (I²C bus based), which counts these pulses for a Time Constant set under the control of embedded code from micro-controller. These counts are interpreted in CPS or CPM or in dose rate (i.e., mR/hr) depending on the mode selected by the user.

Built-in keypad with the following command buttons START, STOP, INC, DEC, STORE, PROG, provide user interface to the instrument. 16x2 LCD dot-matrix display interfaced to the micro-controller displays all the programmed parameters and output results to the user. Built-in EEPROM stores data readings upto 1000. User can store and recall them for later visualization.

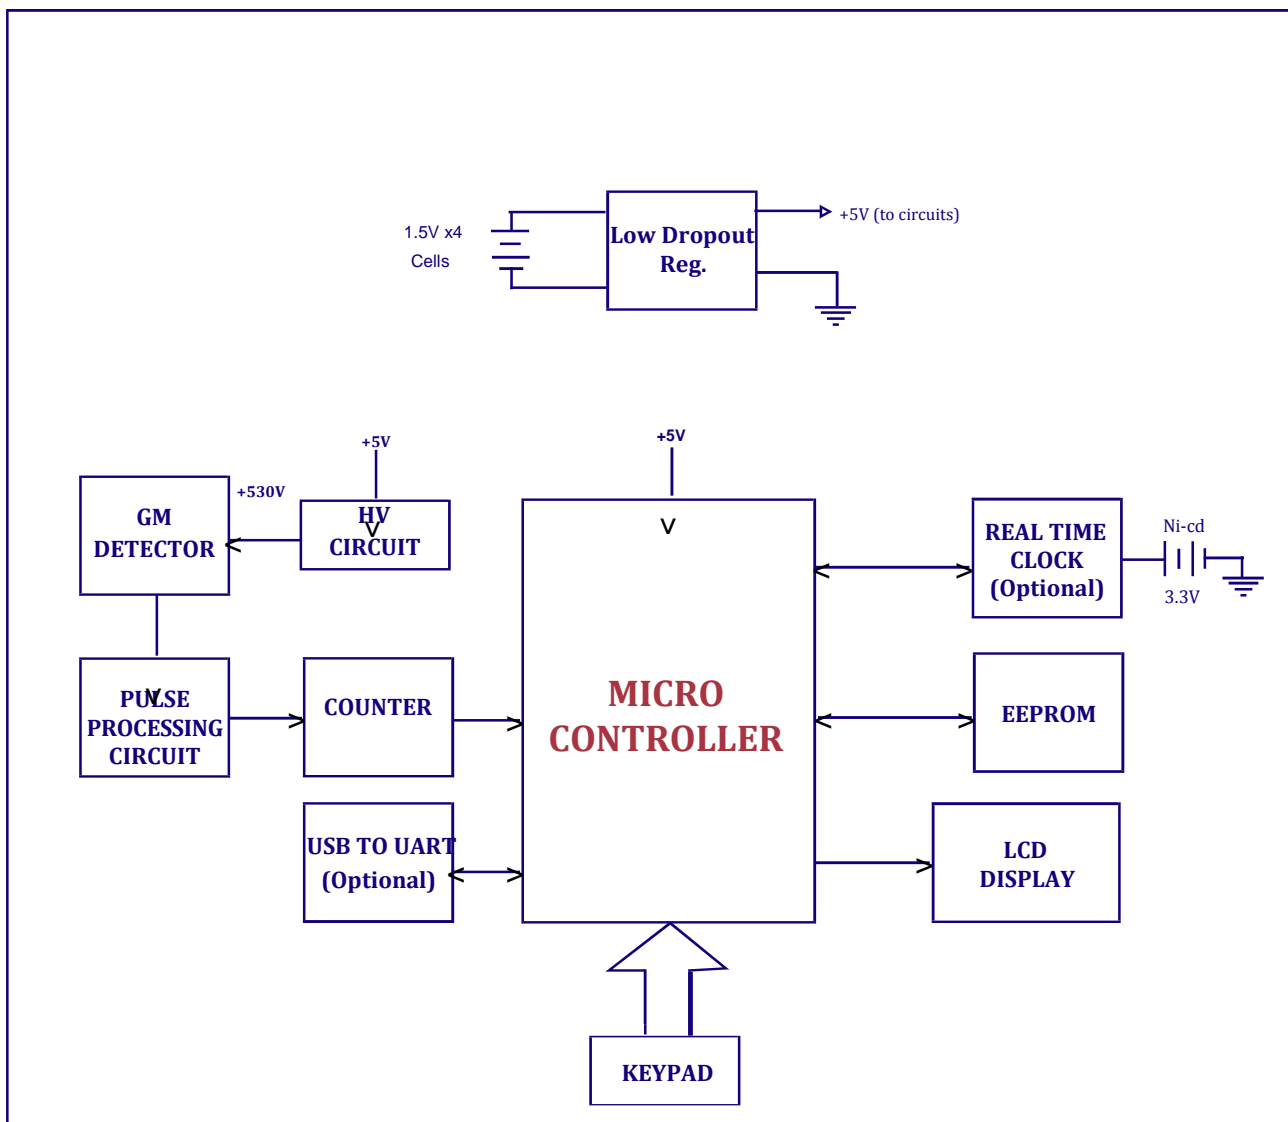

CHAPTER – IX

CONTACT US FOR AVAILING SERVICES

Postal/Mailing Address (Phone / Fax / Email)

Nucleonix Systems Pvt Ltd.
Plot No. 162 A&B, Phase II, I.D.A.,
Cherlapally, Hyderabad - 500 051, Telangana, India.
Phone: + 91-7207034546, 68888777
Mobile: 7331104480, 7331104481, 7331104482
Email : info@nucleonix.com

**For any information, Contact by email is always appreciated.
(This will help us to respond to you quickly)**

Marketing Department:

a) Sales / Commercial Information / Field installation and servicing

For any Commercial, Price information, Product information, customer coordination & quotation of our products customer related commercial services, please contact front office marketing staff through the listed Email Ids or Phone Nos. given below

Whom to Contact:

Business Executives:	Contact Numbers	Contact by E-mail ID
1. R.Maniram (Sr. Business Executive)	Mob: 7331104481, Ph-7207034546	info@nucleonix.com
2. Ch.Gayatri (Business Executive)	Mob: 7331104481, Ph-7207034546	info@nucleonix.com
3. K.Swapna (Business Executive)	Mob: 7331104481, Ph-7207034546	info@nucleonix.com

Note: Our business executives will also connect you to concerned Engineer or General Manager for any technical clarifications if required

b) Factory Services

For **Servicing and Calibration** factory services & follow up on the above jobs including dispatch related/payment related issues of serviced & calibrated items please contact

Ms. K.Sarika
(Executive services)

Mob: 7331104482

E-mail: info@nucleonix.com

She will also connect you to concerned engineer or general manager if required, for any clarifications & deficiencies in services

c) Dispatch Related Issues (Production Items)

For dispatch related issues of your ordered equipment's, including delays, purchase order related document deficiencies, payment proofs, dispatch docket details and bills etc.,contact

Ms.V.Anusha / Renuka
Devi (Executive Dispatch)

E-mail: info@nucleonix.com

d) Product Technical Information / Clarifications

Whom To Contact:

Contact any front office "Business Executive"- He/She will take your details and connect you to concerned product engineer for any technical clarifications. Best thing is to email your technical queries and obtain the reply, rather than on telephone.

You can also contact General Manager or Director (Tech) if required.

e) Marketing Manager

On business matters for all your marketing services / techno commercial requirements about Nucleonix Products contact:

Bhaskara I.V.
Mob:8019662500
Email: info@nucleonix.com

f) General Manager

Dr.M.S.R.Murthy PhD (Nuclear physics)

Email: info@nucleonix.com

Contact General Manager for all sales / servicing and technical information including customer support related issues, on the delays, gaps & lapses by our staff. Contact G.M. regarding field installations & field servicing jobs schedule etc.

g) H.R -Incharge

Contact her regarding, job vacancies, sending resume for employment, H.R. related issues etc. contact

Ms. Shanthi Sri . P

Mob:7331104480

Email: recruit@nucleonix.com

h) Director -Technical

Mr. J. Dheeraj Reddy

Email: jdreddy@nucleonix.com

Mobile No: +91-7674009005

Contact him for, any Technical Information and clarifications on products, which cannot be answered by General Manager / Customer support executives.

For any technical deficiencies in products, related issues & suggestions on product improvements you may contact by email or telephone. This will help the company to improve the product & serve you better.

Dealer's complaints, on commercials, lapses by our commercial staff, or any other discrepancy, or you like to give any feedback on any Nucleonix staff doing any wrong thing against cleaner / ethical business principles / practices can be complained to any of the directors or managing director.

i) Director - IT

Mr. J. Nishanth Reddy

Email: nishureddy@yahoo.com, info@nucleonix.com

Mobile No. +91-9966691000

For any deficiencies in product software's, related issues, & any suggestions or improvisations in software's can be contact by email or telephone. This will help the company to improve the product & serve you better.

j) Managing Director

Shri. J.Narender Reddy (Managing Director)

Email : jnreddy@nucleonix.com, info@nucleonix.com

Contact Managing Director for, Foreign relations, International Business co-operation, Joint ventures, Exports, Dealership in other countries, Policy matters, Technology tie-ups etc.

k) Dealers Complaints :

Dealers complaints, on commercials, lapses by our commercial staff, or any other discrepancy, or you like to give any feedback on any Nucleonix staff doing any wrong thing against cleaner / ethical business principles / practices can be complained to any of the directors or managing director.

**An innovative company working towards excellence
in the field of Nuclear Instrumentation**



NUCLEONIX SYSTEMS PVT. LTD.

Plot No.162 A & B, Phase-II, IDA, Cherlapally, Hyderabad-500051 INDIA.

Ph : + 91-7207034546, + 91-7331104481, 7331104482.

E-mail : info@nucleonix.com website : www.nucleonix.com